



COLOQUICK

TEAT + ESOPHAGEAL TUBE FEEDER ASSEMBLY GUIDE

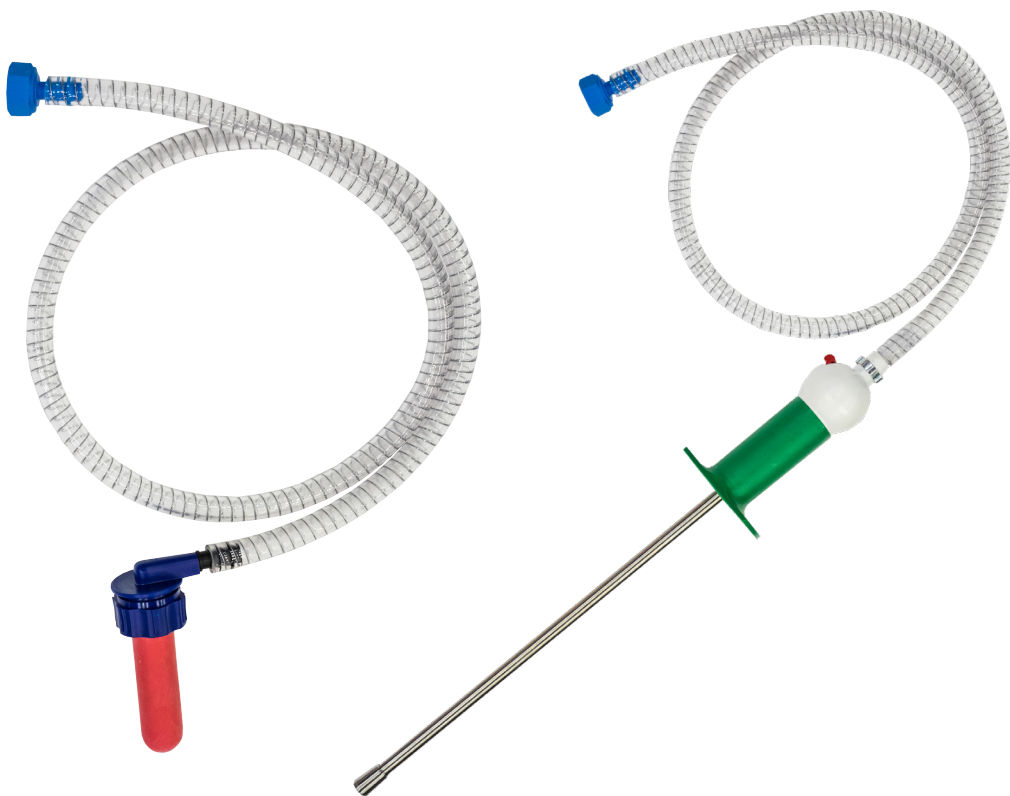

1 Mount the hose connector and the complete teat onto the hose, one in each end.

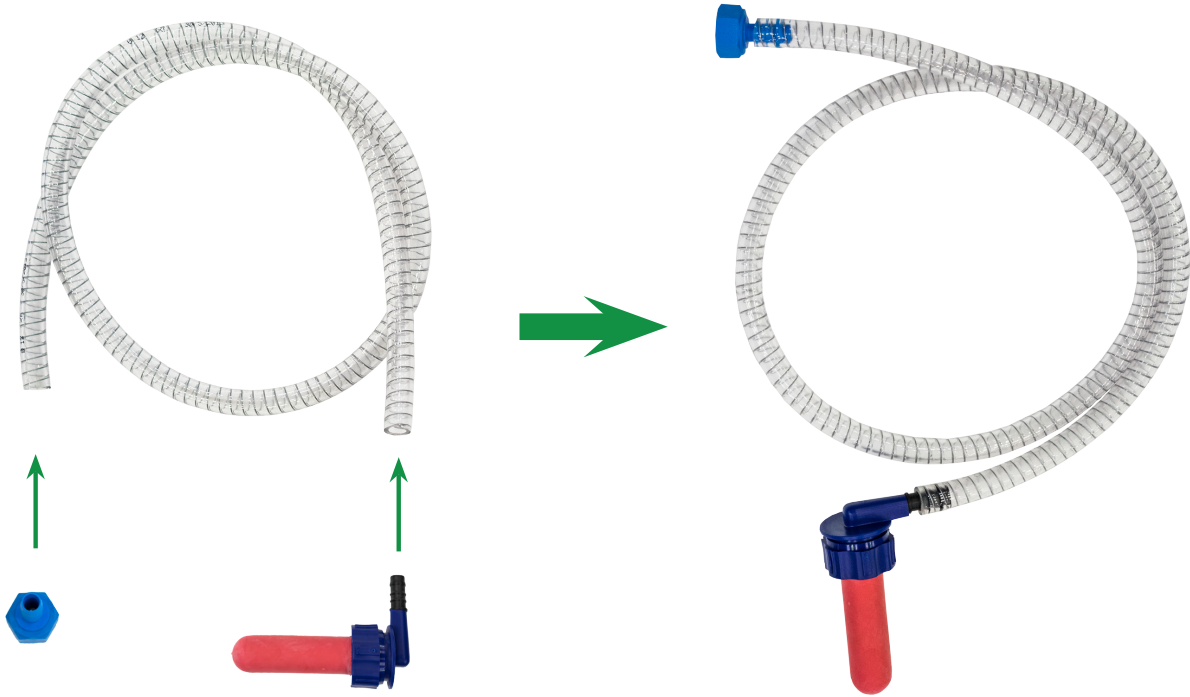

2 Mount the hose connector and the esophageal tube feeder device onto the hose, one in each end.

